



Work Together

Item Code 73036

Infrared Thermometer with Dual Laser Pointer E Emissivity Adjustable Model

Instruction Manual

Introduction

Thank you for purchasing the Shinwa Infrared Thermometer with Dual Laser Pointer E Emissivity Adjustable Model. Before using the product, please read the instructions contained in this manual to ensure correct use. After having read this manual, always keep it with you or in a safe place.

■ Specifications

Accuracy	0 - 550°C: $\pm 2\%$ or 2°C (higher value) -60 - 0°C: $\pm \{-2 + (\text{displayed value} \times 0.05)\}$ °C
Measuring Range	-60 - 550°C
Resolution	-9.9 - 199°C: 0.1°C Other values: 1°C
Measuring Interval	1 sec
Operating Temperature	0 - 50°C
Emissivity	Adjustable 0.1 - 1 (default as 0.95)
Auto Power Off	60 seconds after stopped operation
Battery Life	14 hours (continuous use)*1
Power Source	2x AAA Alkaline batteries (Batteries included are for trial use only and may not last as long)
Laser Wavelength	635 - 660 nm
Output	1 mW or less (JIS Class2)
Dust/Waterproof	IP54*2
Body Size	144 × 43 × 117 mm
Weight	180 g (with battery)
Material	Body: ABS resin, elastomer resin

*1 When the laser pointer and backlight are not on, the device can be used continuously for 140 hours

*2 5 Dustproof performance: A small amount of dust that has penetrated inside will not hinder normal operation.

4 Waterproof performance: It will not be harmfully affected by a splash of water from any direction.

■Part Names

●Body

LCD panel

Displays the temperature measured as well as other related information.

Infrared lens

(detects infrared rays)

Detects the infrared rays emitted by the object being measured.

▼ switch

MODE switch

▲ switch

Measurement switch

Temperature is measured while the switch continues to be pressed.

Dual laser

light-emitting ports

2 points of red laser light show both sides of the measuring range diameter.

Battery cover

2x AAA alkaline batteries (Batteries included are for trial use only and may not last as long.)

●LCD panel

Laser pointer icon

Turns on when laser pointer is set to ON, and flashes while laser is active.

Battery icon

Displays the amount of battery power remaining.

HOLD icon

Turns on after temperature is measured while in HOLD Measurement mode.

Temperature display

Displays the temperature measured. Displays every 0.1°C from -9.9°C up to less than 200°C while no decimal points will be displayed for other measurement values.

Backlight icon

Turns on when backlight is set to ON.

LOCK icon

Turns on while in LOCK Measurement mode.

Illustration on the left is an example display of maximum temperature measured

Current temperature: 123.4°C

Maximum temperature: 135.7°C

Maximum Temperature Display Mode



Mode display




Displays the current mode.

Sub display

Displays necessary information in each mode.

■ Changing the Battery


The thermometer will not work when the battery is low. We recommend immediately replacing with new AAA alkaline batteries. Open the battery cover, and insert 2x AAA batteries in the correct position.

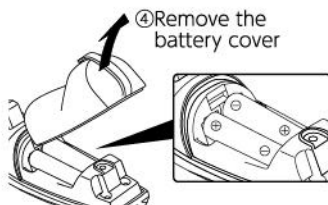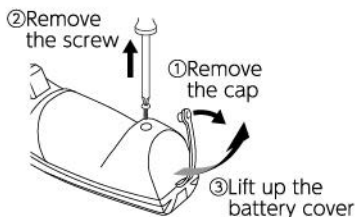

Removing the batteries will cause the device to return to the following default settings.


Default setting

Laser pointer	: OFF
Backlight	: OFF
Hold measurement mode	: ON
Emissivity(E)	: 0.95
MAX, MIN, dIF, AVG	: No value
HAL	: 550
LAL	: -60



The mode and other settings will be retained even if the device automatically turns off.

■ Measurement Distance and Range

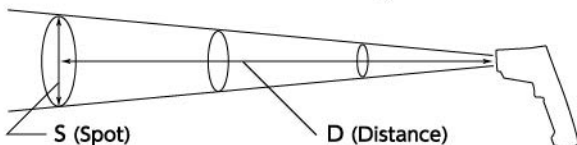

[Distance coefficient] $D \text{ (Distance)} : S \text{ (Spot)} = 12 : 1$

Example: 24 cm distance to the object being measured → 2 cm spot
6 m distance to the object being measured → 50 cm spot

*Measuring range minimum diameter: 20 mm

■About This Device and Emissivity

This device is a non-contact thermometer which reads the infrared rays emitted from an object, converts them to temperature, and displays them on the LCD panel.

The emissivity of infrared rays will differ depending on the object. To take an accurate measurement of temperature, it is necessary to match this device with the emissivity of the object.

The emissivity of a mirrored surface or an object through which light passes will be strongly affected by reflectivity and transmittance. To take an accurate measurement of temperature, please measure after first affixing black-body tape or coating with a black-body paint.

Emissivity Chart


Measured Object	Emissivity
Water/ice	0.98
Soil	0.92 - 0.96
Stone/asbestos	0.92
Plastic	0.90 - 0.95
Rubber (black color)	0.95
Wood	0.98

Measured Object	Emissivity
Paper	0.92
Vegetables/fruit	0.98
Meat	0.98
Copper oxide	0.5 - 0.6
Iron oxide	0.7 - 0.8
Tile	0.8



*Emissivity may differ slightly depending on factors such as the temperature of the object measured, the condition of its surface, and its color. Please use the Emissivity Chart above only as a reference.

■How to Set Emissivity

- ① Press the MODE switch several times and go to the Start Screen shown below (E will be shown).
 - ② From the Start Screen press the MODE switch once, and go to the Set Emissivity Screen. (*E_▲ will be shown).
- *The initial setting is 0.95 emissivity.
- ③ Press the ▲ switch or the ▼ switch and set the emissivity. Press the MODE switch to change out of this mode and finalize the setting.



Start Screen



Set Emissivity Screen

*Values displayed will vary with the settings.

■ Before Using

● Power ON/OFF

The device can be turned ON by pressing the Measurement switch or the MODE switch.

The power will turn off (Auto Power Off) after 60 seconds pass without operation while in HOLD Measurement mode.

Auto Power Off is disabled while in LOCK Measurement mode.

● Laser pointer ON/OFF

Pressing the ▼ switch while simultaneously pressing the Measurement switch turns the laser pointer ON or OFF. The laser pointer icon (▲) will be displayed when the laser is set to ON, and laser light will be irradiated from the laser light-emitting port while the Measurement switch is pressed.

● Backlight ON/OFF

Pressing the ▲ switch while simultaneously pressing the Measurement switch turns the backlight ON or OFF. The backlight icon (☼) is displayed while the backlight is ON.

■ How to Measure

Point the device's measuring window toward the object to be measured, and take a reading of the temperature on the display.

■ Measurement Modes

● HOLD Measurement mode

In this mode, the temperature will be continuously measured while the Measurement switch is pressed, and when it is released the temperature will remain fixed.


● LOCK Measurement mode

This mode allows continuous measurement regardless of whether the Measurement switch is pressed or not.

① When pressing the Measurement switch and turning on the power, the LCD panel will display HOLD, and the device will be in HOLD Measurement mode.

② Pressing the ▲ switch when the mode display is *E*, *MAX*, *MIN*, *dIF*, or *AVG* changes the device to LOCK Measurement mode, and LOCK will be displayed on the LCD panel. Press the ▲ switch again to return to HOLD Measurement mode.

*Changing mode is not possible when the mode display is *°E*, *HRL*, or *LAL*.

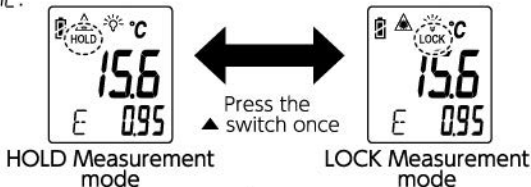

■ Maximum Temperature / Minimum Temperature / Difference Between Max and Min Temperature / Average Temperature

Pressing the MODE switch from the Start Screen (page 4) allows the device to switch between different types of temperature display.

● Maximum temperature display

- ① From the Start Screen (E will be shown), press the MODE switch 2 times, and *MAX* will be displayed.
- ② The maximum temperature measured will be displayed from when the Measurement switch is first pressed to when it is released.



32.3
MAX 47.8

● Minimum temperature display

- ① From the Start Screen (E will be shown), press the MODE switch 3 times, and *MIN* will be displayed.
- ② The minimum temperature measured will be displayed from when the Measurement switch is first pressed to when it is released.



32.3
MIN 19.5

● Difference between max and min temperature

- ① From the Start Screen (E will be shown), press the Mode switch 4 times, and *dIF* will be displayed.
- ② The difference between the maximum temperature and the minimum temperature measured will be displayed from when the Measurement switch is first pressed to when it is released.



32.3
dIF 28.3

● Average temperature

- ① From the Start Screen (E will be shown), press the MODE switch 5 times, and *AVG* will be displayed.
- ② The average temperature will be displayed from when the Measurement switch is first pressed to when it is released.



32.3
AVG 33.4

■HI/LOW Alarm Functions*1

●HI Alarm*2

- ①From the Start Screen (E will be shown), press the MODE switch 6 times, and *H_{AL}* will be displayed.
- ②Set the alarm temperature with the ▲/▼ switches.
- ③When a temperature higher than the one set in the alarm is measured, the device will notify you with a buzzer.



●LOW Alarm*2

- ①From the Start Screen (E will be shown), press the MODE switch 7 times, and *L_{AL}* will be displayed.
- ②Set the alarm temperature with the ▲/▼ switches.
- ③When a temperature lower than the one set in the alarm is measured, the device will notify you with a buzzer.



*1 If the HI alarm and/or LOW alarm are not needed, return them to their default setting.

*2 When both the HI alarm and LOW alarm are set, the buzzer will sound for each setting.

■Troubleshooting

Hi	Outside measurement range (higher than 550°C)
	Measure a temperature cooler than 550°C.
Lo	Outside measurement range (lower than -60°C)
	Measure a temperature that is warmer than -60°C.
Er2	Rapid change in temperature
	Measure after the device has adjusted to the ambient temperature.
Er3	Outside operating temperature range (lower than 0°C or higher than 50°C)
	Measure after the device has sufficiently adjusted to its operating temperature range.
Er	Other error messages
	After removing the batteries and waiting for at least 1 minute, reinsert them, then turn the device on and try measuring again.

The thermometer requires at least 30 minutes to adjust to the ambient temperature. For all other error messages, it is necessary to reset the thermometer. To reset it, turn the device off, remove the batteries and wait for at least 1 minute, then reinsert the batteries and turn on. Please contact us if the error message remains.

Warning

- Never look at the laser source directly or point the laser at others. The laser light could cause vision loss if it directly enters the eye.
- Keep the thermometer out of the reach of children.

Caution

- Do not use the thermometer as a clinical thermometer.
- The device is not resistant against water. Do not use in an area where it could get wet, as this could damage it.
- Do not disassemble or alter the device, as this may lead to malfunctioning.
- Do not drop or subject to strong impact as this may cause the device to operate incorrectly.
- Keep the measuring window (the part that detects infrared rays) clean. To clean it, wipe with a soft cloth or cotton fabric dampened in water or alcohol for medicinal use (ethyl alcohol). Measurements taken while the device is wet could cause malfunction, so make sure that it is dry before using.
- Note that steam, dust, and smoke can affect the accuracy of the temperature measurement.
- Remove the battery before storing the device when not being used for a long period.
- This is a non-contact infrared thermometer. Do not allow it to touch the object being measured. Contact with an object at a very high temperature may cause a mistaken measurement to be displayed or cause the device to break down.
- See the ■ Specifications section for details about the accuracy of this device. For temperature control that requires greater accuracy, please purchase a precision thermometer.
- Measurement differences may occur depending on factors such as material, luster, thickness, color and emissivity of the object.
- When using the device in an environment with electronic noise, the display could become unstable or there may be significant errors. Also, do not bring the thermometer close to electrified objects.
- Do not wash or wipe the device with alcohol, thinner, or any other organic solvent. To wipe dirt away, soak a gauze or similar fabric with neutral detergent in lukewarm water and wipe only after thoroughly wringing out the cloth. Do not allow the gauze or fabric to make direct contact with the temperature measuring part.
- A rapid change in the ambient temperature may affect the accuracy. Use the device after it has sufficiently adjusted to the ambient temperature. In the case that the ambient temperature changes by more than 10°C, it will take the device more than 30 minutes to adjust to it.
- We shall not be liable for any consequential, incidental, or indirect damages such as losses and lost profits to the customer as well as a third party resulting from the operation of this product, regardless of whether or not they were foreseeable or the possibility was reasonably foreseeable. However, this shall not apply in the case where there is willful or gross negligence or when the customer is a consumer according to the Consumer Contract Act. In the event that we are liable for the use of this product, we shall be liable for damages limited to an amount equal to the price of the product.